


**Patient:** Barry Hills  
**Recorded:** Tuesday, April 29, 2025 at 2:01:04 PM  
**Heart Rate:** 60 BPM  
**Duration:** 30s

**Kardia Determination:** Possible Atrial Fibrillation  
\*Kardia Determination is done on Lead I.


Enhanced Filter, Mains Frequency: 60Hz Scale: 25mm/s, 10mm/mV

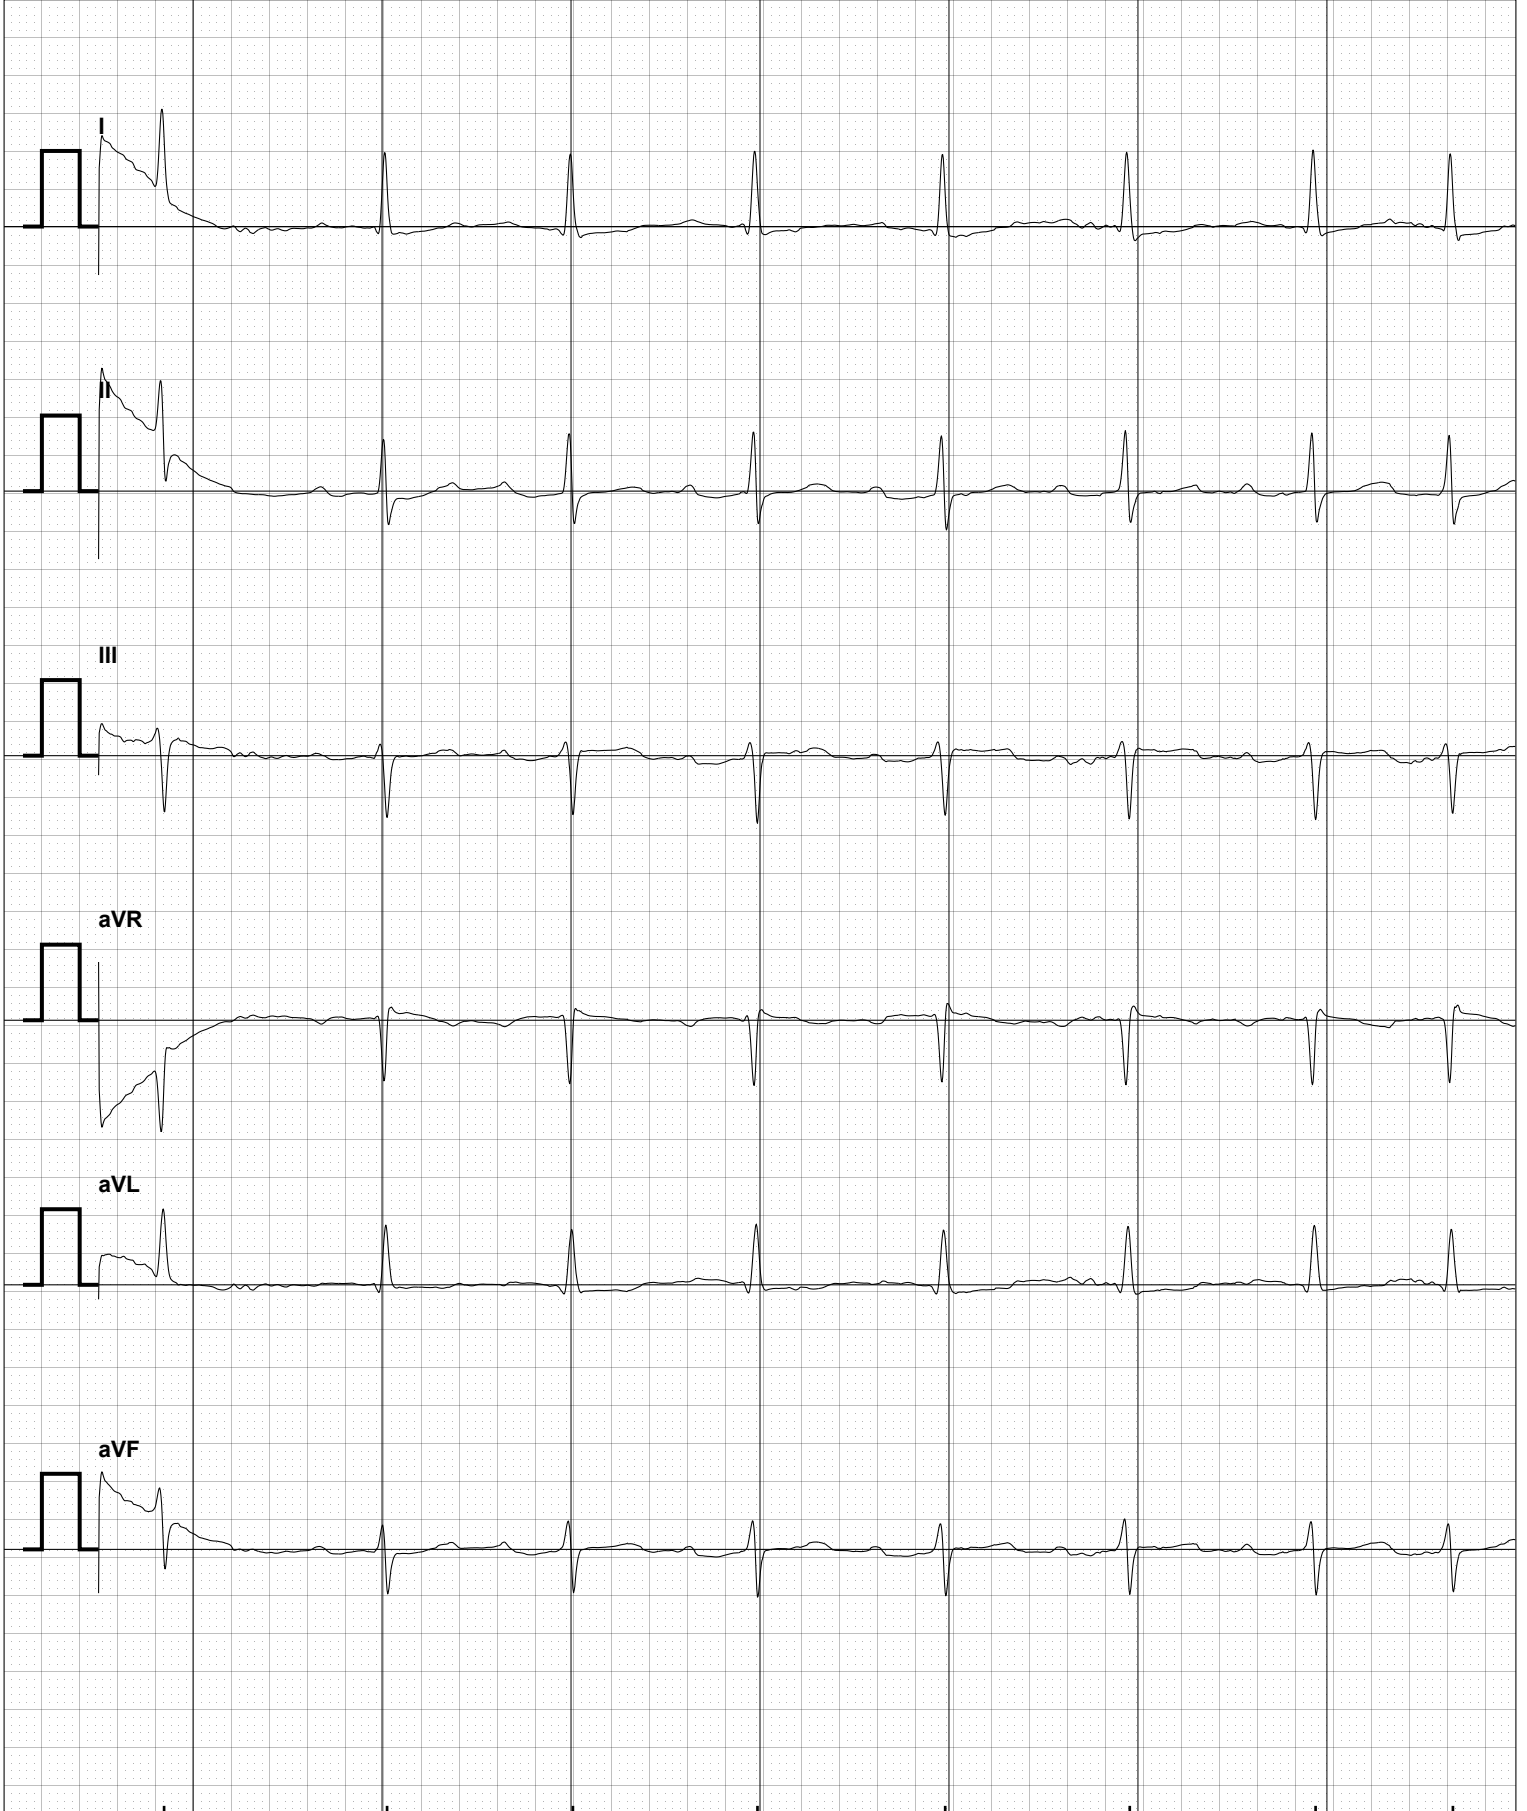

**Patient:** Barry Hills  
**Recorded:** Tuesday, April 29, 2025 at 2:01:04 PM  
**Heart Rate:** 60 BPM  
**Duration:** 30s

**Kardia Determination:** Possible Atrial Fibrillation  
\*Kardia Determination is done on Lead I.


Enhanced Filter, Mains Frequency: 60Hz Scale: 25mm/s, 10mm/mV

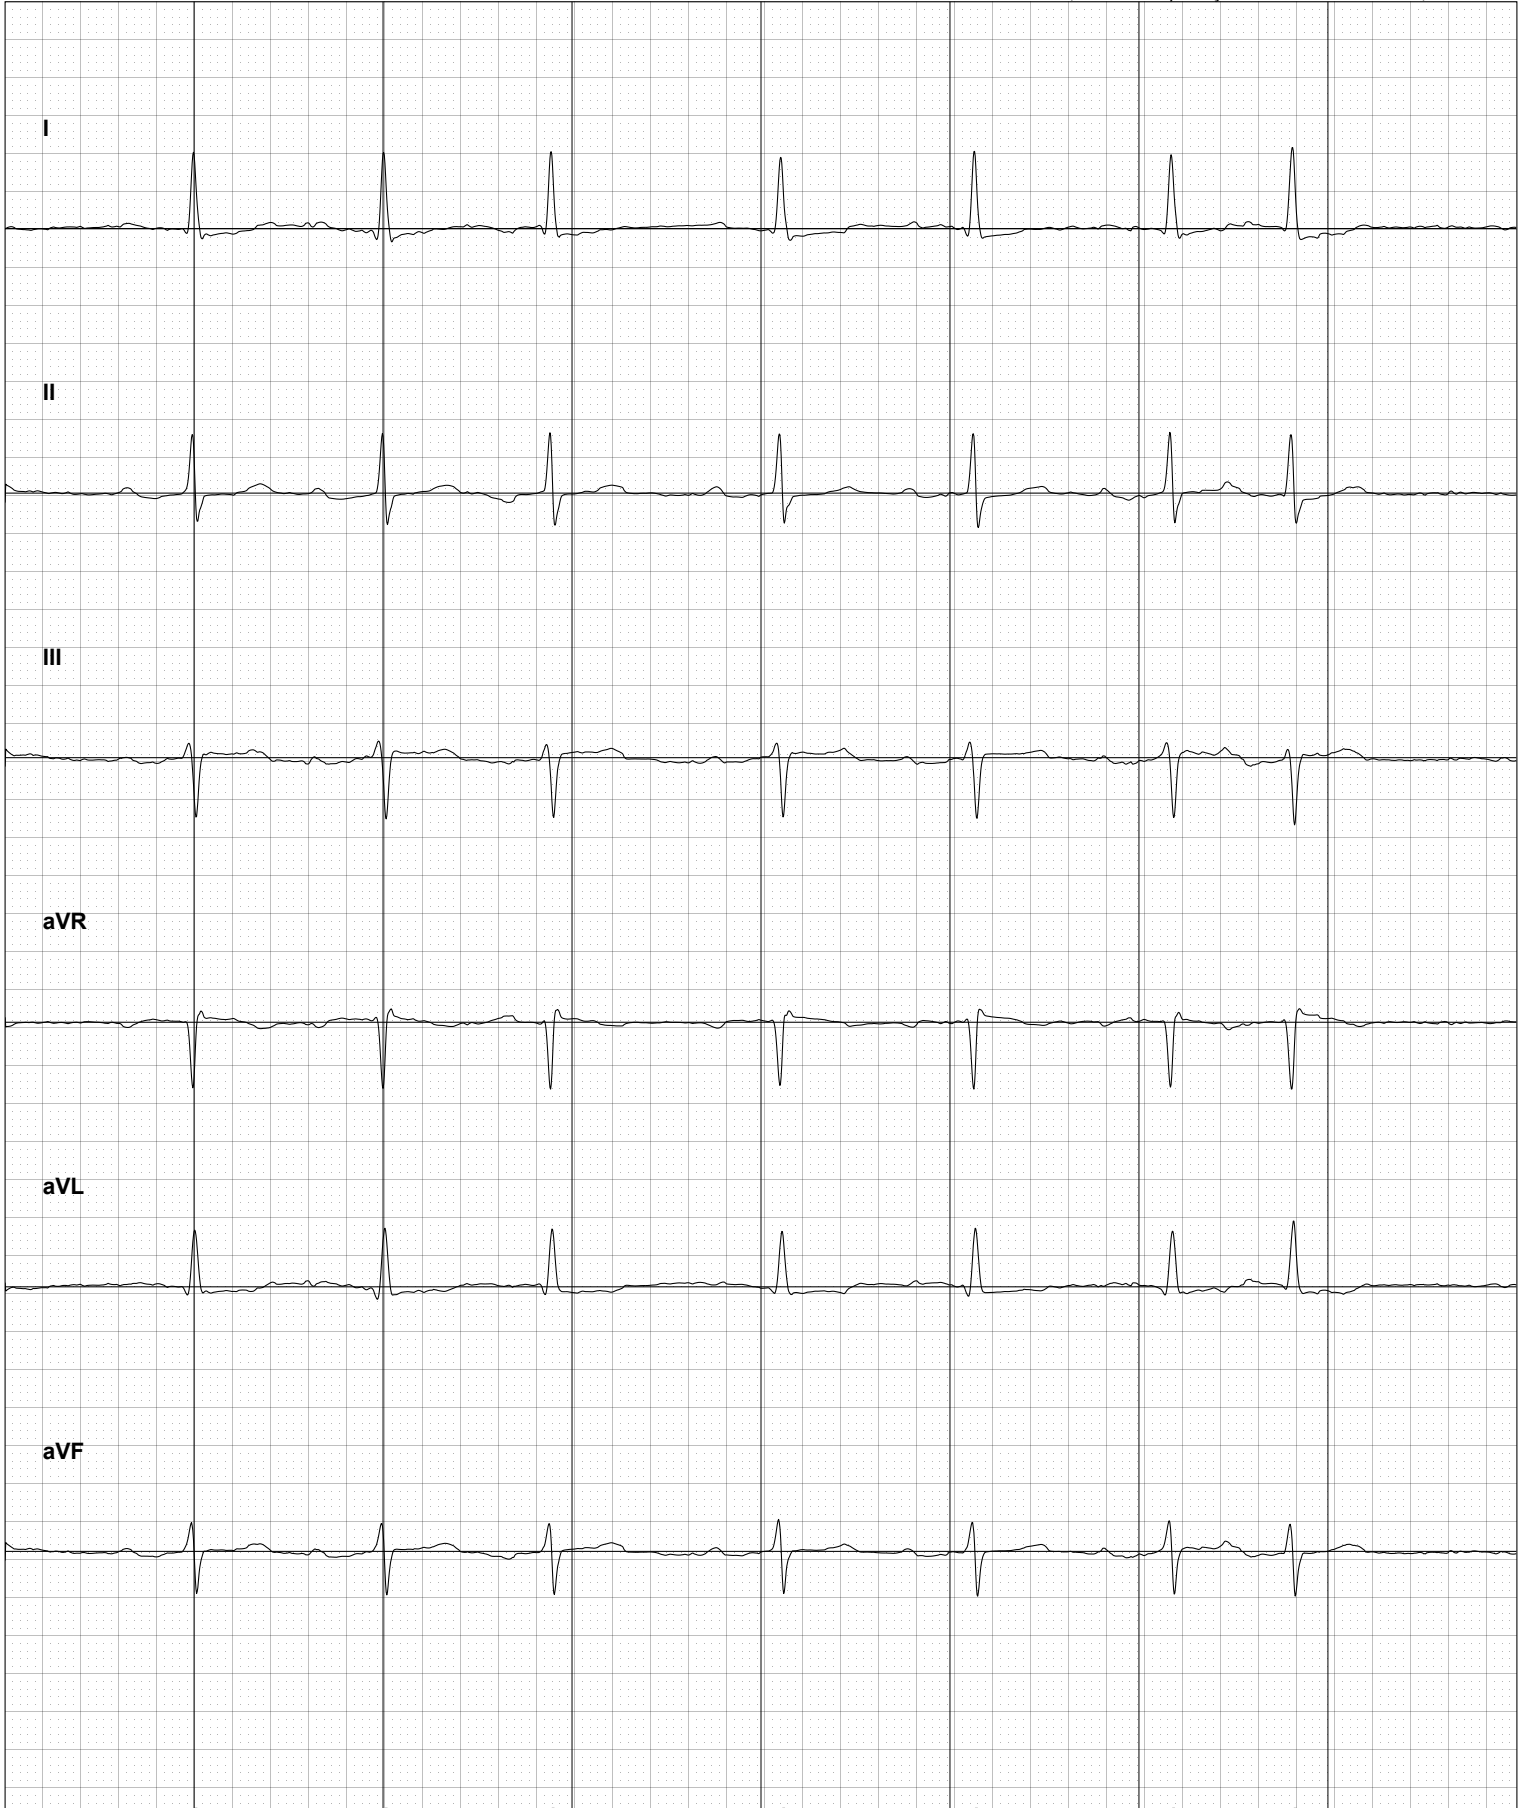

**Patient:** Barry Hills  
**Recorded:** Tuesday, April 29, 2025 at 2:01:04 PM  
**Heart Rate:** 60 BPM  
**Duration:** 30s

**Kardia Determination:** Possible Atrial Fibrillation  
\*Kardia Determination is done on Lead I.

Enhanced Filter, Mains Frequency: 60Hz Scale: 25mm/s, 10mm/mV

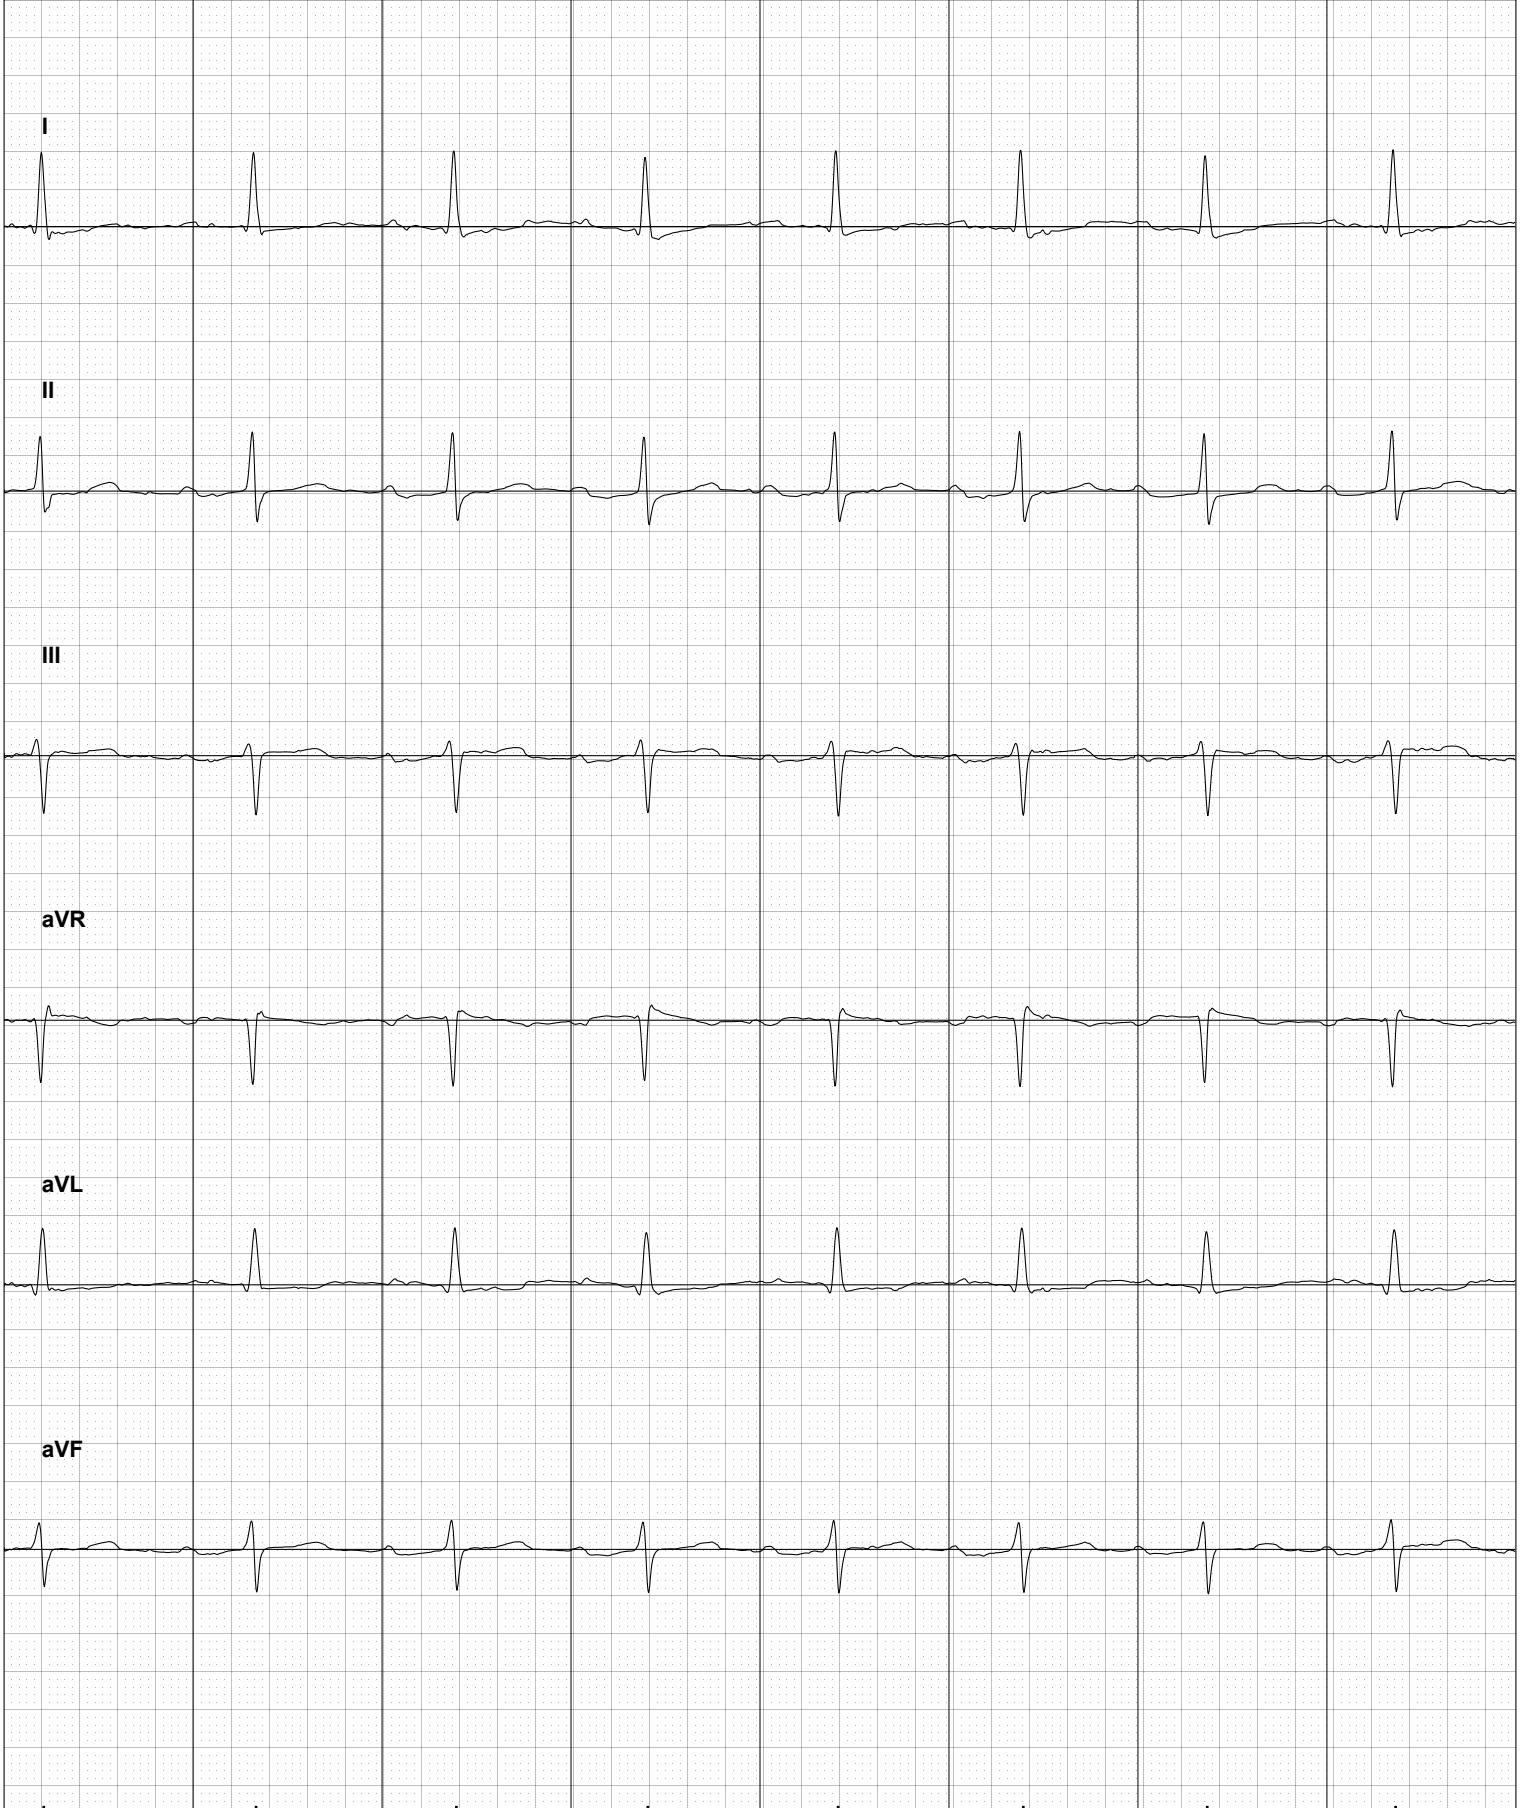

**Patient:** Barry Hills  
**Recorded:** Tuesday, April 29, 2025 at 2:01:04 PM  
**Heart Rate:** 60 BPM  
**Duration:** 30s

**Kardia Determination:** Possible Atrial Fibrillation  
\*Kardia Determination is done on Lead I.

Enhanced Filter, Mains Frequency: 60Hz Scale: 25mm/s, 10mm/mV

