


**Patient:** Barry Hills  
**Recorded:** Wednesday, August 20, 2025 at 5:37:38 AM  
**Heart Rate:** 58 BPM  
**Duration:** 30s

**Kardia Determination:** Possible Atrial Fibrillation  
\*Kardia Determination is done on Lead I.


Enhanced Filter, Mains Frequency: 60Hz Scale: 25mm/s, 10mm/mV

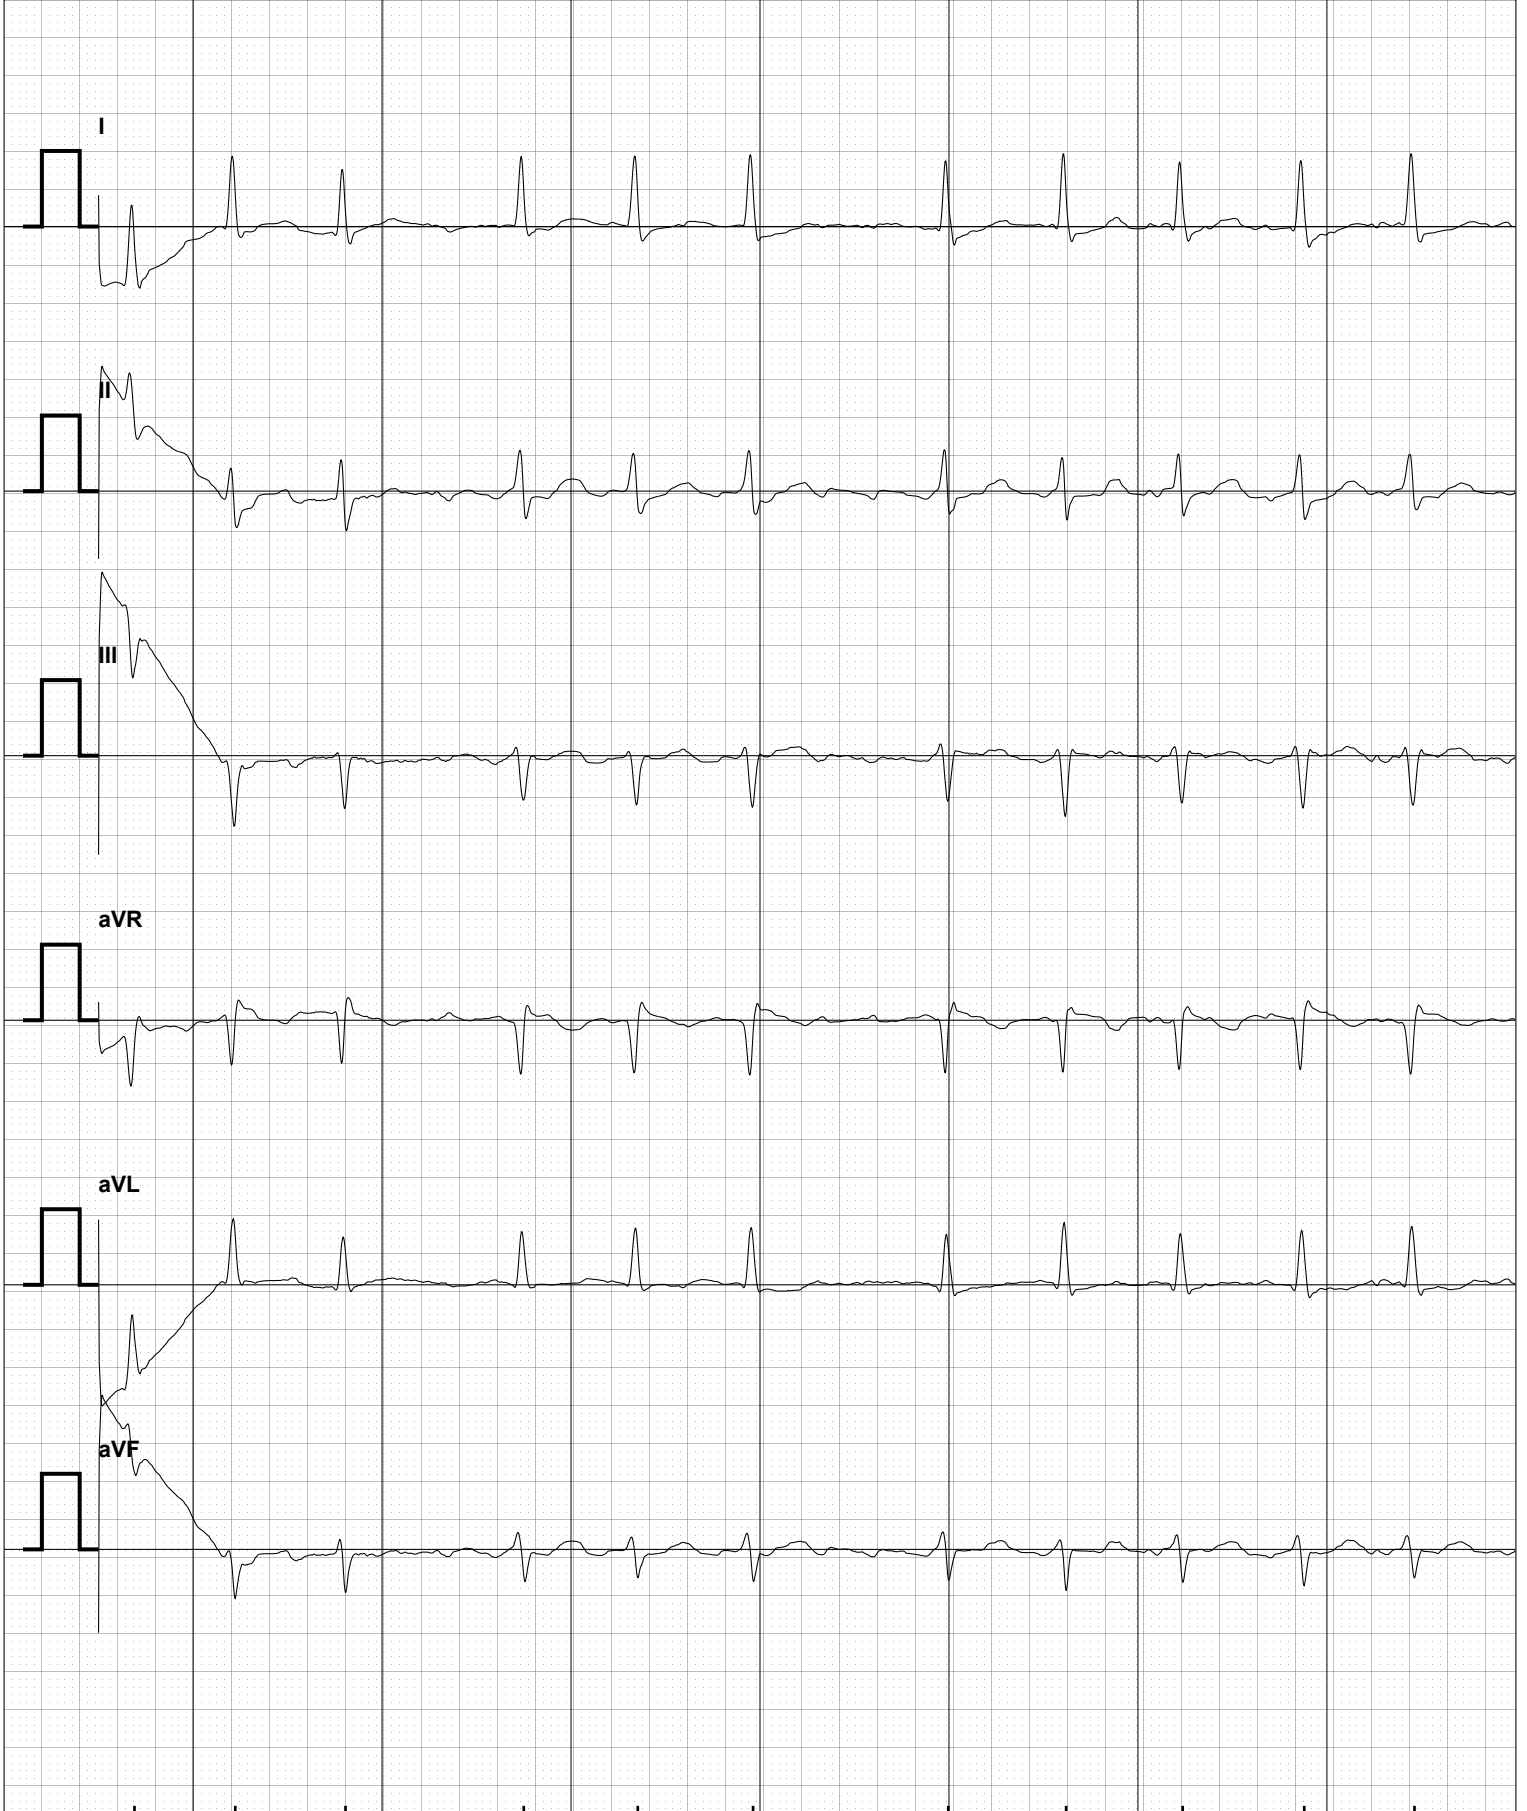

**Patient:** Barry Hills  
**Recorded:** Wednesday, August 20, 2025 at 5:37:38 AM  
**Heart Rate:** 58 BPM  
**Duration:** 30s

**Kardia Determination:** Possible Atrial Fibrillation  
\*Kardia Determination is done on Lead I.


Enhanced Filter, Mains Frequency: 60Hz Scale: 25mm/s, 10mm/mV

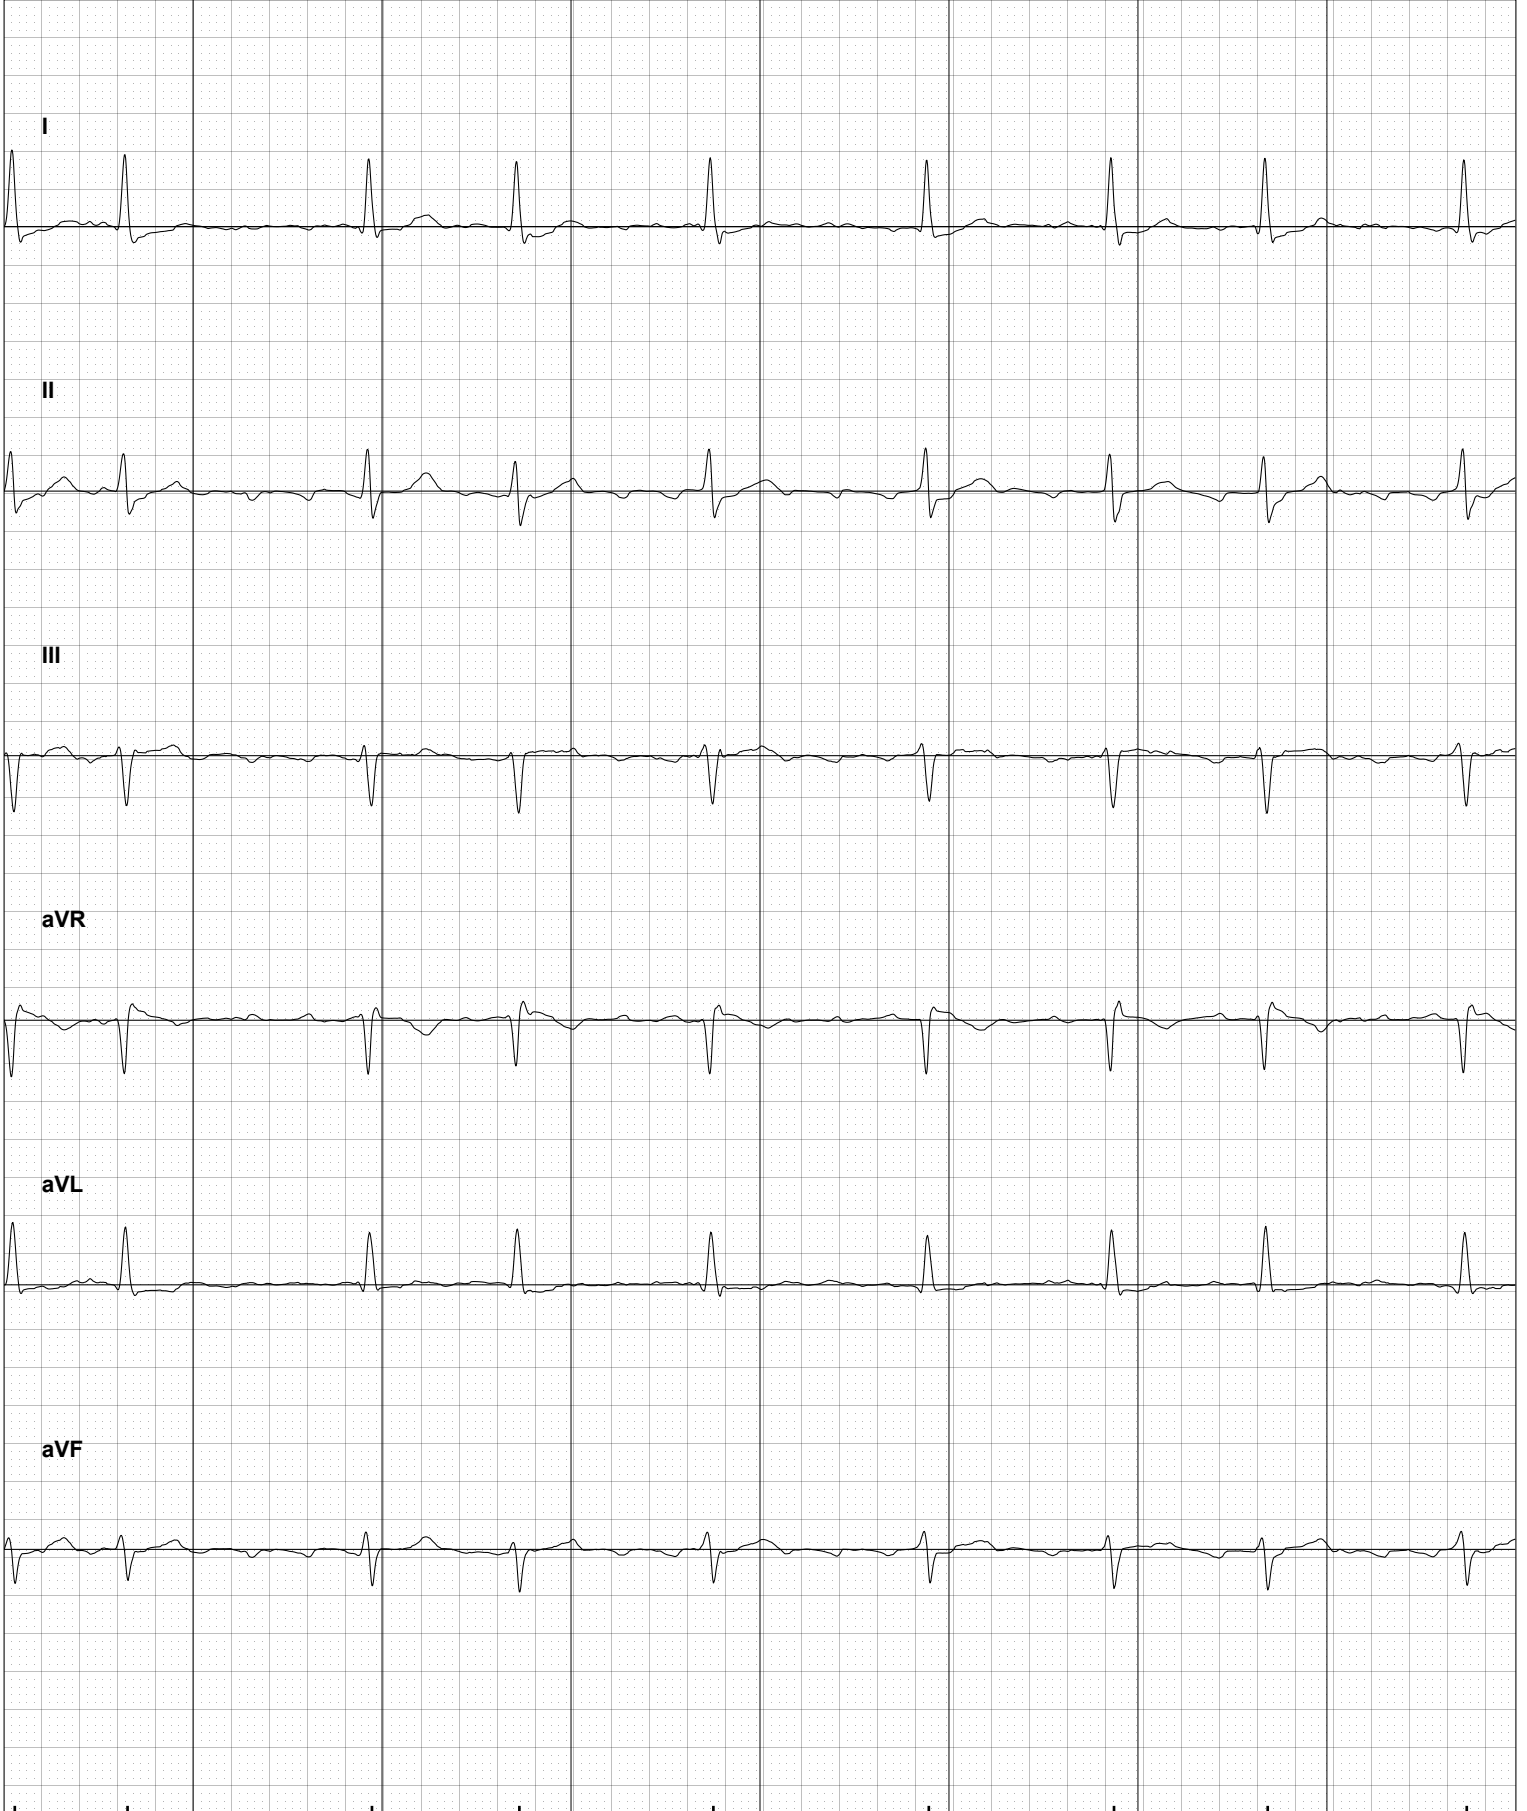

**Patient:** Barry Hills  
**Recorded:** Wednesday, August 20, 2025 at 5:37:38 AM  
**Heart Rate:** 58 BPM  
**Duration:** 30s

**Kardia Determination:** Possible Atrial Fibrillation  
\*Kardia Determination is done on Lead I.

Enhanced Filter, Mains Frequency: 60Hz Scale: 25mm/s, 10mm/mV

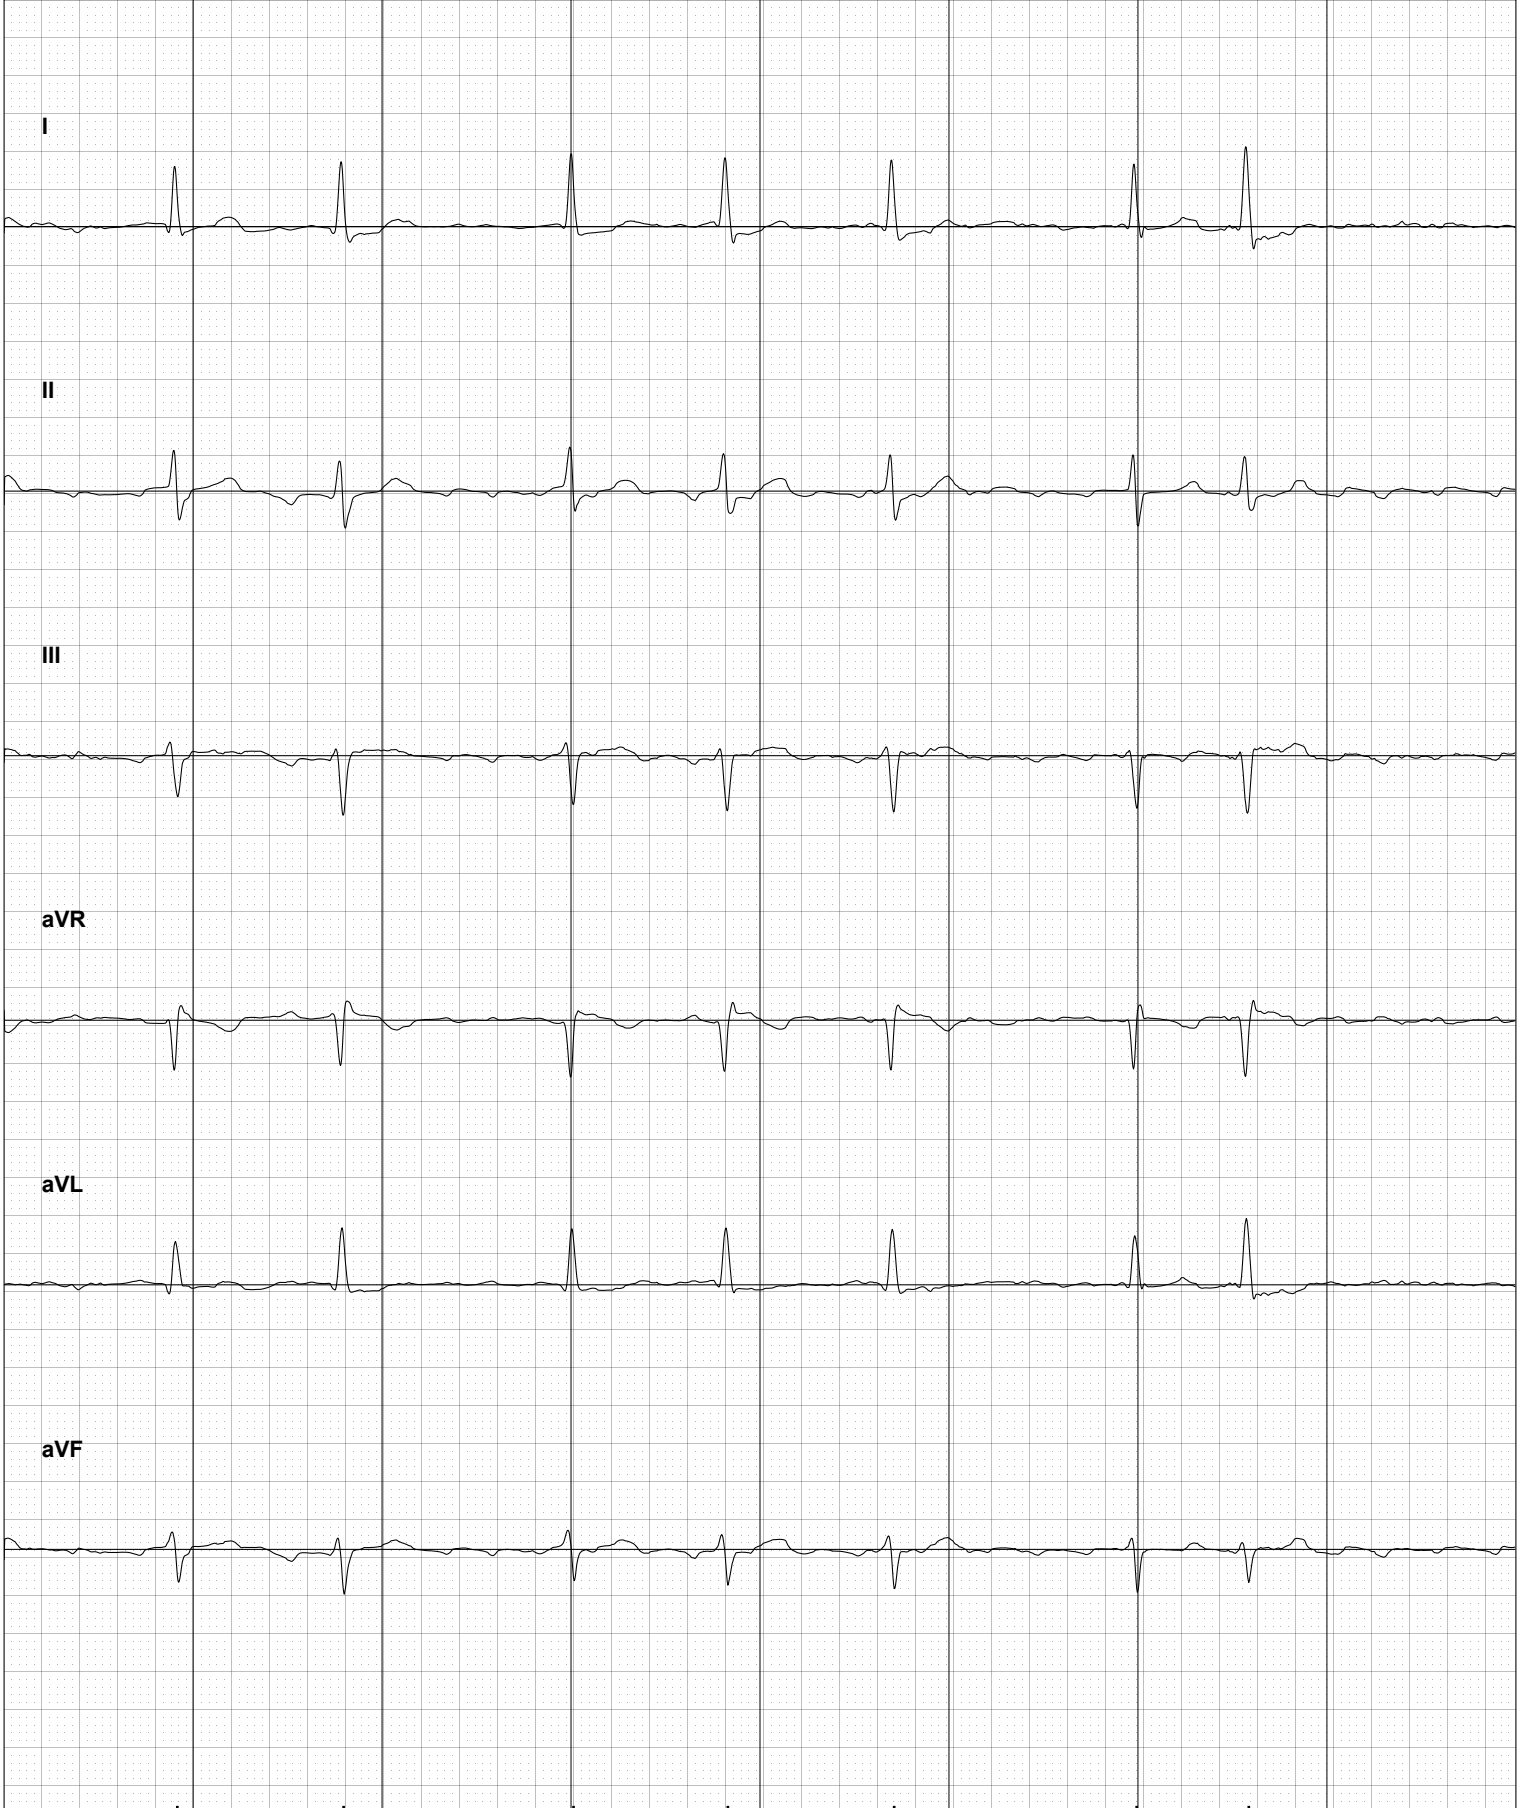

**Patient:** Barry Hills  
**Recorded:** Wednesday, August 20, 2025 at 5:37:38 AM  
**Heart Rate:** 58 BPM  
**Duration:** 30s

**Kardia Determination:** Possible Atrial Fibrillation  
\*Kardia Determination is done on Lead I.

Enhanced Filter, Mains Frequency: 60Hz Scale: 25mm/s, 10mm/mV

