

Patient: Barry Hills
Recorded: Saturday, September 6, 2025 at 6:28:33 PM
Heart Rate: 66 BPM
Duration: 30s

Kardia Determination: Possible Atrial Fibrillation
*Kardia Determination is done on Lead I.


Enhanced Filter, Mains Frequency: 60Hz Scale: 25mm/s, 10mm/mV



Patient: Barry Hills
Recorded: Saturday, September 6, 2025 at 6:28:33 PM
Heart Rate: 66 BPM
Duration: 30s

Kardia Determination: Possible Atrial Fibrillation
*Kardia Determination is done on Lead I.

Enhanced Filter, Mains Frequency: 60Hz Scale: 25mm/s, 10mm/mV

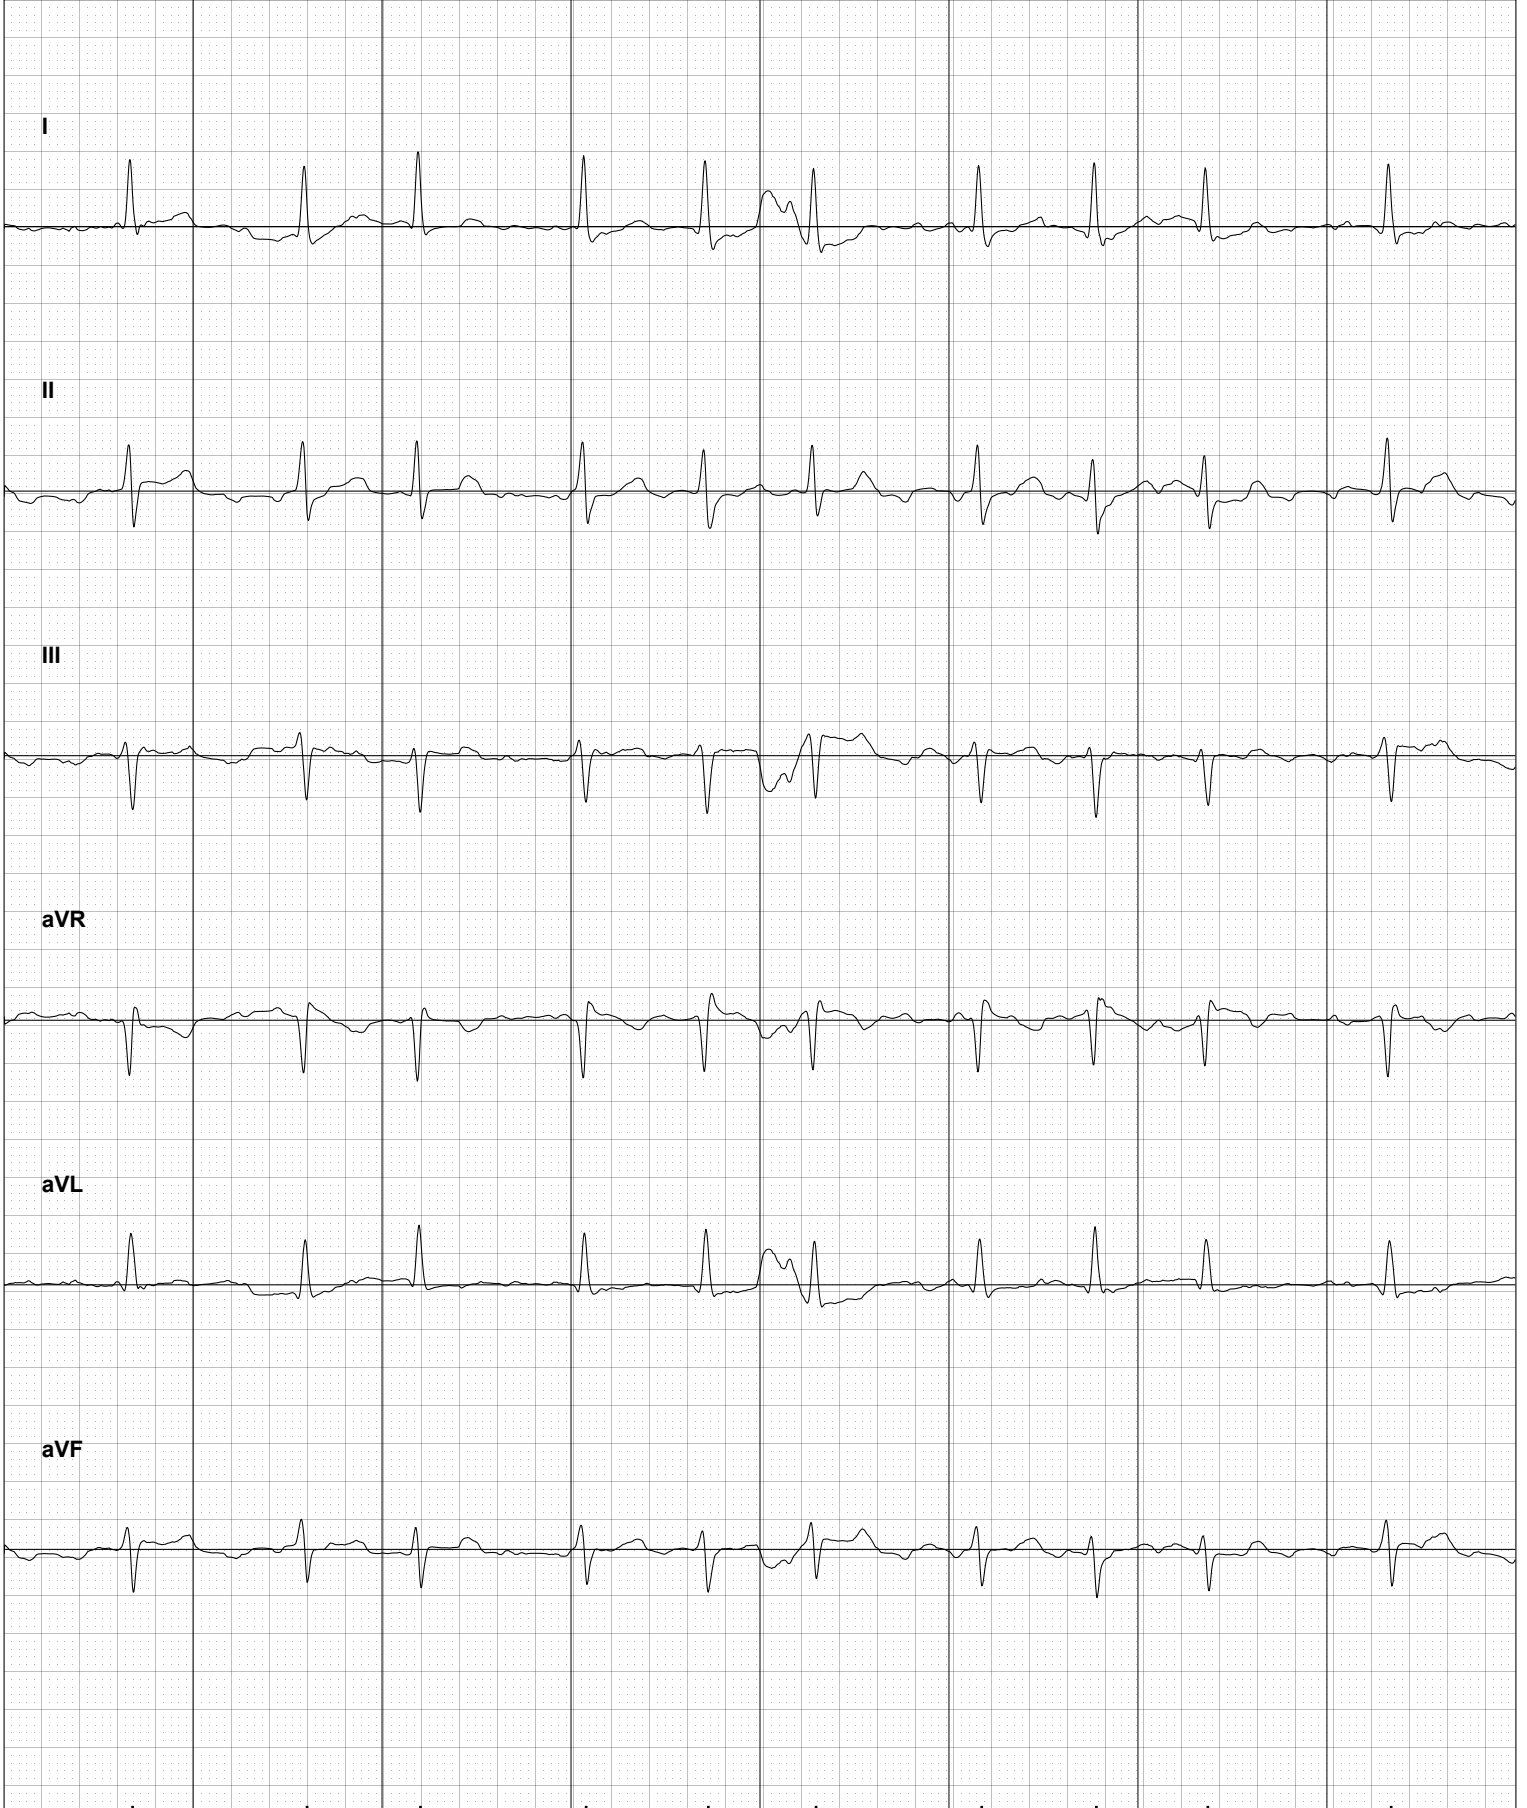

Patient: Barry Hills
Recorded: Saturday, September 6, 2025 at 6:28:33 PM
Heart Rate: 66 BPM
Duration: 30s

Kardia Determination: Possible Atrial Fibrillation
*Kardia Determination is done on Lead I.

Enhanced Filter, Mains Frequency: 60Hz Scale: 25mm/s, 10mm/mV

